ANALIZA BIAŁEK

Scan for verify

100018120

Laboratory of Analysis

Client: Vitasynlab
Order number: 100018120
Name: VS VITASYNLAB BPC-157
Number of samples: 1 vial

Batch number: ------
Receive date: 2026-09-07
Start date: 2026-09-09
End date: 2026-09-25

Sample identification

Substance	Method of taking a sample	Form
BPC-157	Sample provided by customer	White powder in a glass vial

Results

Test	Sample name	Result
TYMC	VS VITASYNLAB BPC-157 10MG	PASS
TAMC	VS VITASYNLAB BPC-157 10MG	PASS
Presence of presumptive Escherichia Coli	VS VITASYNLAB BPC-157 10MG	NOT DETECTED
Presence of Salmonella Spp.	VS VITASYNLAB BPC-157 10MG	NOT DETECTED

Heavy metal	Sample name	Result
Arsenic	VS VITASYNLAB BPC-157 10MG	<0,010mg/kg
Cadmium	VS VITASYNLAB BPC-157 10MG	0,098mg/kg
Lead	VS VITASYNLAB BPC-157 10MG	0,297mg/kg
Mercury	VS VITASYNLAB BPC-157 10MG	<0,010mg/kg

Password

CPUNIYRM

Analiza Bialek sp. z o.o.
KRS: 0000966168
NIP: 8992922970
REGON: 521751875

Headquarters and Laboratory:
ul. Duńska 9, 54-427 Wrocław
Budynek DELTA


Lab technician:
Analysis and research specialist
mgr Arkadiusz Zając

ANALIZA BIAŁEK

Scan for verify

100018120

Photo of the test sample

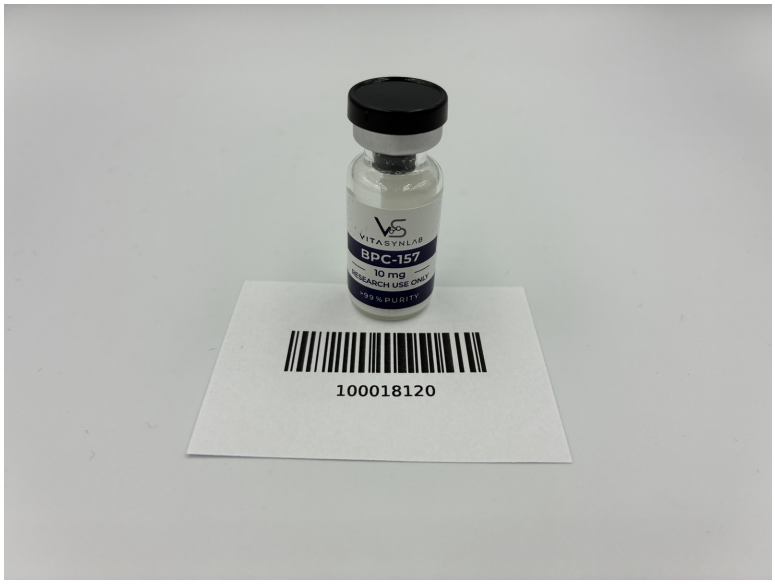

Password

CPUNIYRM

Analiza Bialek sp. z o.o.
KRS: 0000966168
NIP: 8992922970
REGON: 521751875

Headquarters and Laboratory:
ul. Duńska 9, 54-427 Wrocław
Budynek DELTA

Lab technician:
Analysis and research specialist
mgr Arkadiusz Zając