ANALIZA BIAŁEK

Scan for verify

100018119

Laboratory of Analysis

Client: Vitasynlab
Order number: 100018119
Name: VS VITASYNLAB TIRZEPATIDE
Number of samples: 1 vial

Batch number: ------
Receive date: 2026-09-07
Start date: 2026-09-09
End date: 2026-09-25

Sample identification

Substance	Method of taking a sample	Form
Tirzepatide	Sample provided by customer	White powder in a glass vial

Results

Test	Sample name	Result
TYMC	VS VITASYNLAB TIRZEPATIDE 10MG	PASS
TAMC	VS VITASYNLAB TIRZEPATIDE 10MG	PASS
Presence of presumptive Escherichia Coli	VS VITASYNLAB TIRZEPATIDE 10MG	NOT DETECTED
Presence of Salmonella Spp.	VS VITASYNLAB TIRZEPATIDE 10MG	NOT DETECTED

Heavy metal	Sample name	Result
Arsenic	VS VITASYNLAB TIRZEPATIDE 10MG	<0,010mg/kg
Cadmium	VS VITASYNLAB TIRZEPATIDE 10MG	0,099mg/kg
Lead	VS VITASYNLAB TIRZEPATIDE 10MG	0,301mg/kg
Mercury	VS VITASYNLAB TIRZEPATIDE 10MG	<0,010mg/kg

Password

ETL5W3SC

Analiza Bialek sp. z o.o.
KRS: 0000966168
NIP: 8992922970
REGON: 521751875

Headquarters and Laboratory:
ul. Duńska 9, 54-427 Wrocław
Budynek DELTA


Lab technician:
Analysis and research specialist
mgr Arkadiusz Zając

ANALIZA BIAŁEK

Scan for verify

100018119

Photo of the test sample

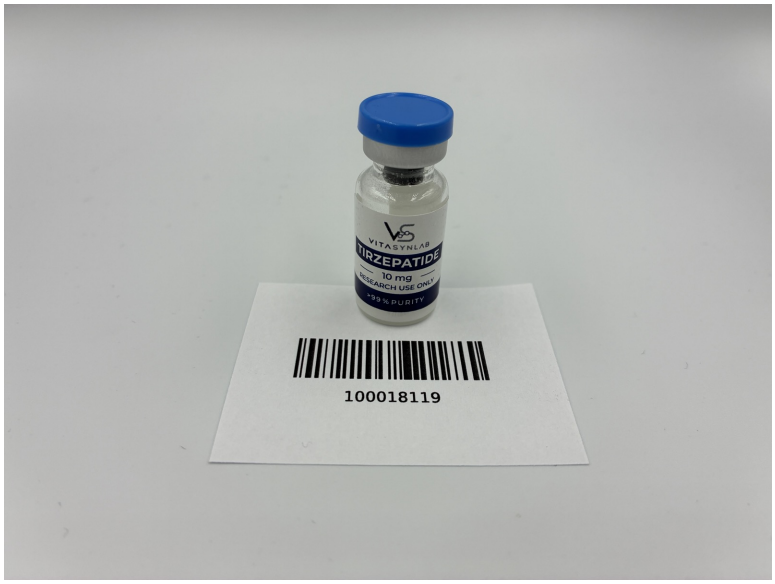

Password

ETL5W3SC

Analiza Bialek sp. z o.o.
KRS: 0000966168
NIP: 8992922970
REGON: 521751875

Headquarters and Laboratory:
ul. Duńska 9, 54-427 Wrocław
Budynek DELTA

Lab technician:
Analysis and research specialist
mgr Arkadiusz Zając